



EU REPRESENTATIVE / IMPORTER: Nissha Medical Technologies SAS 25 Boulevard de la Paix 95800 Cergy, France +33 1 39 72 66 66




HS.NisshaMedical.com


ECG DIAGNOSTIC ELECTRODE

FOR USE WITH:

| Product No | Reference No | Product No | Reference No | Product No | Reference No |
|-------------------|---------------------|-------------------|--------------|-------------------|---------------------|
| 6500015V | A10005-3-7% | 6500581V | A10071-5NB | 6500060V | A10040-60 |
| 6500017V | A10005-7%NB | 6502754V | A10096SG-30 | 6500061V | A10041-60 |
| 6500019V | A10005-60-7% | 6502779V | A10097-3 | 6500062V | A10042-10 |
| 6500021V | A10005SG-60 | 6502781V | A10097-5 | 6500064V | A10042-60 |
| 6500049V | A10031-1-60 | 6502782V | A10097-5NB | 6502683V | Z05MC-3 |
| 6500051V | A10031-60 | 6502785V | A10097-7NB | 6502684V | Z05MC-5 |
| 6500484V | A10005SG-30 | 6500070V | A10070-1-60 | 6502685V | Z05MC-50 |
| 6502801V | A10098-10NB | 6500071V | A10070-5 | 6502687V | Z05MT-3 |
| 6500636V | A10098-30 | 6500023V | A10006-3 | 6502688V | Z05MT-5 |
| 6502789V | A10098-5NB | 6502776V | A10006-60 | 6502689V | Z05MT-50 |
| 6500057V | A10033-1-60 | 6500028V | A10006-60T | 6502692V | Z05SG-3 |
| 6500053V | A10032-1-60 | 6502843V | P7-3 | 6502693V | Z05SG-30 |
| 6500054V | A10032-5 | 6500003V | A10000-60 | 6502694V | Z05SG-5 |
| 6500055V | A10032-60 | 6500004V | A10001 | 6502695V | Z05SG-50 |
| 6500048V | A10026T-60 | 6502842V | A7-5 | 6502721V | Z35-3 |
| 6502954V | A10005SG-5NB | 6502769V | A10040-5 | 6502722V | Z35-5 |
| 6502947V | A10005SG-3NB | 6502767V | A10041-5 | 6502723V | Z35-50 |
| 6500072V | A10071-1-60 | 1 | | l | |

INSTRUCTIONS FOR USE

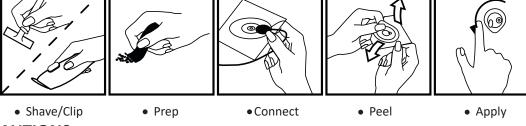



CAUTIONS

- Federal law restricts this device to sale by or on the order of a physician.
- ECG electrodes should only be used by or in consultation with a health care provider familiar with their proper placement and use;
- ECG electrodes may damage the skin if removed carelessly;
- ECG electrodes should be applied only to intact, clean skin (e.g., not over open wounds, lesions, infected, or inflamed areas); and
- ECG electrodes should be properly disposed of after use
- Minor skin irritation can occur with electrode use. If skin irritation occurs, please contact your prescribing physician or health care professional.

PRECAUTIONS

- During surgical procedures, electrodes should be placed as far as possible from any electro-surgical area to minimize unwanted RF
- Self-adhesive electrodes should be replaced if they no longer stick firmly to the skin.

VMI 174 (04/2021)





















